

MEASURES THE VISCOSITY OF A HYDROCARBON LIQUID STREAM

The Model 1077 small bore Viscometer is a completely automatic process stream analyser for measuring viscosity in absolute units. When used with a density measurement, correlation with ASTM D 445 can be achieved.

TYPICAL APPLICATIONS

The analyser is suitable for use with **Newtonian** samples which are not sensitive to shear rate.

- Lube oil blending
- Fuel oil blending
- Lube oil de-waxing
- Distillate fuel product specification
- Visbreaker feed stock

PRINCIPLE OF OPERATION

The analyser measures differential pressure across a capillary through which a fluid is passed. The differential pressure is proportional to the absolute viscosity of the fluid as described by the Hagan-Poiseuille equation:

$$\mu = \frac{1.45 \times 10^5 \times d^4 P}{QL}$$



where μ = absolute viscosity in centiPoise (cP)
 d = capillary bore (mm)
 P = differential pressure across capillary (bar)
 Q = sample flow (ml/min)
 L = capillary length (mm)

as d , Q and L are constants, μ (absolute viscosity) is directly proportional to P (differential pressure measured across capillary).

A precision pump meters the flow of sample. To ensure that the sample metered by the pump is at approximately at the same temperature as the sample entering the capillary, two heat exchangers are fitted, one either side of the metering pump. Input pressure is set so that the metering pump suction pressure is always positive.

The sample flows at a constant rate through the capillary, across which a differential pressure transmitter is connected. The output of this pressure transmitter is then directly proportional to the absolute viscosity of the sample.

The critical components are maintained at a fixed temperature by immersion in an oil bath, the temperature of which is controlled by a precision temperature controller, heater and, when necessary, water cooling. The temperature is monitored by the relevant ASTM (IP) thermometer. The capillary is housed in an easily removable holder to enable cleaning or range changing without needing to lower the bath.

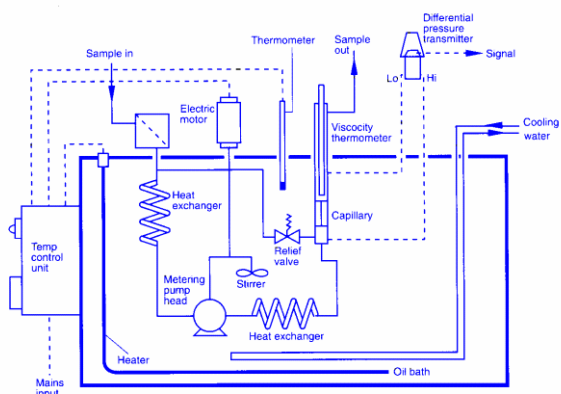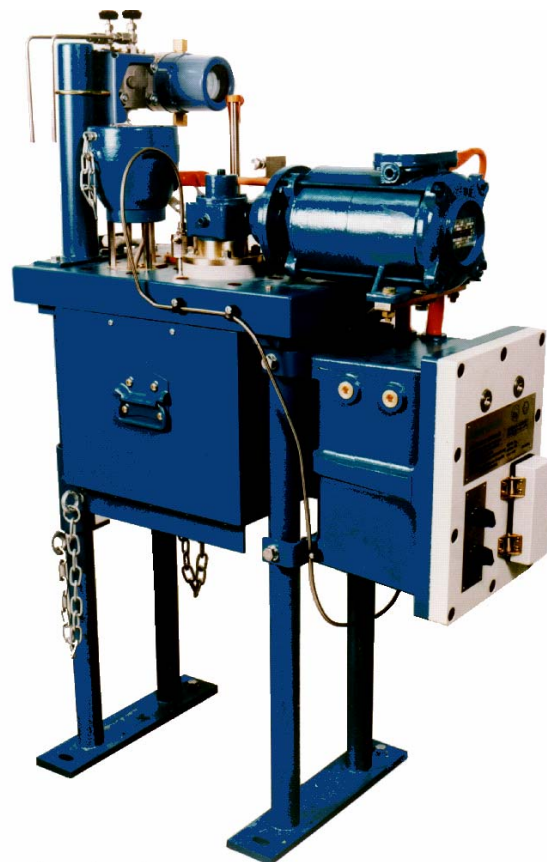

ONE OF THE ATAC RANGE OF PROCESS ANALYSERS

SPECIFICATION

Analysers performance

Ranges	By capillary selection Maximum : 0 - 2500cP Minimum : 0 - 5cP
Repeatability	± 0.5% FS.
Precision	± 1% FS.
Response time	30 seconds to 3 minutes depending on sample temperature

Specified measurement temperature

Normally 40 - 150°C (100 - 300°F) but 170°C is available (see options).

Output signal

Range	4 - 20 mA fully isolated loop powered.
or	Digital output depending on transmitter selected

Out-of-service alarm contact signalling mains failure (or off) or bath temperature fuse blown.

Sample conditions required at inlet

Pressure	Within range 0.7 - 21 bar g (10 - 304 psig) dependent upon the viscosity of sample.
Temperature	Must be within ±100°C (212°F) of the required measuring temperature.
Flow	60.7 ml/min (0.8 gal/h) when power supply frequency is 50Hz and 72.8 ml/min (0.9 gal/h) at 60Hz.

Sample conditioning

Sample should be clean and filtered prior to being introduced into the analyser. Pressure pulses should be avoided.

The analyser will accept samples having the above inlet conditions. Complete sample systems can be supplied to condition sample as required at the analyser inlet.

Sample disposal

Return to process or a recovery system. Sample recovery systems can be supplied.

Utility requirements

Power supply

Voltage	115V or 230V ± 10% single phase
Frequency	50 or 60 Hz
Consumption	1.5 kVA or 2.0 kVA depending on the specified measurement temperature.

Cooling water

When the sample is at a high temperature or when the measurement temperature is low with respect to ambient, a supply of cool, potable water (9 - 45 l/h) should be provided to carry away the excess heat. The necessary coil is fitted as standard. If potable water is not available, alternative cooling coil materials can be provided.

Steam for tracing

Steam at low pressure (1 bar max) will be required for samples having a pour point above lowest ambient temperature.

Oil for temperature bath

11 litres (2.5 gal) of Shell Thermia B or equivalent. Normal maximum working temperature of bath is 150°C (protected by a thermal fuse). The sample temperature at capillary outlet is measured by a mercury-in-glass thermometer.

Local display

0 - 100% linear scale on the transmitter.

Standard connections

Sample in	1/4" NPT (female)
Sample outlet	3/8" NPT (female)
Cooling water	1/4" NPT (female) IN
Cooling water	1/4" NPT (female) OUT

Electrical M25 (power), M20 (alarm)
(1/2" NPT NEC)

Signal out As transmitter specification
either EExd or EExia with
4-20mA isolated output or
digital output.

Steam tracing 1/4" o.d. compression

Explosion protection

Model 1077J The analyser is ATEX certified
II 2G EEx d e IIB T1-T6*
*model dependent
for use in zone 1 areas.
Certificate no.
EPSILON 04SYS1283V1

Model 1077H Explosion proof design for
use in NEC Class 1,
Groups C & D, Div 1 Area.

Model 1077F CSA Certified
Exd e IIB T3
Class 1, Zone 1

Environmental protection

The Viscometer is free-standing and, provided that it is sheltered from direct sun, rain and strong winds, it will operate satisfactorily outdoors under normal temperature conditions in the range 0 - 55°C (32 - 130°F).

Dimensions and weight

Width	490 mm
Depth	860 mm
Height	1270 mm
Weight	195 kg

Floor fixing bolt holes (4 off 5/8" dia) at
441 mm (17 5/8") x 351 mm (13 13/16")
centres.

Access dimensions

Length	1680 mm
Depth	1550 mm (inc.open door)
Height	1830 mm

The space below the viscometer must be kept clear for lowering the oil bath.

Options

- Steam tracing and lagging of transmitter for high pour point samples. Transmitter is enclosed in traced metal box. Bleed connectors are brought out to external valves. Impulse lines are traced and lagged (fitted as required).
- Local digital indicator (scaled in engineering units).
- Water cooled gearbox and high temperature stirrer. These items when fitted allow operation of the viscometer at up to 170°C.
- Digital transmitter with integral microprocessor permitting remote diagnostics, configuration and interrogation of transmitter plus loop integrity test using manufacturer's hand-held communicator.
- Measurement of viscosity at line temperature.
- Remote indication of bath temperature.

1077 JAN 2004

For further information contact :-



Analytical
Technology
& Control
Limited

Unit 6, Redlands Centre,
Coulson, Surrey, CR5 2HT,
England.
Telephone:+44 (0)208 763 9494
Fax:+44 (0)208 763 9540
E-mail:atac@atacuk.com